

EXHIBIT P

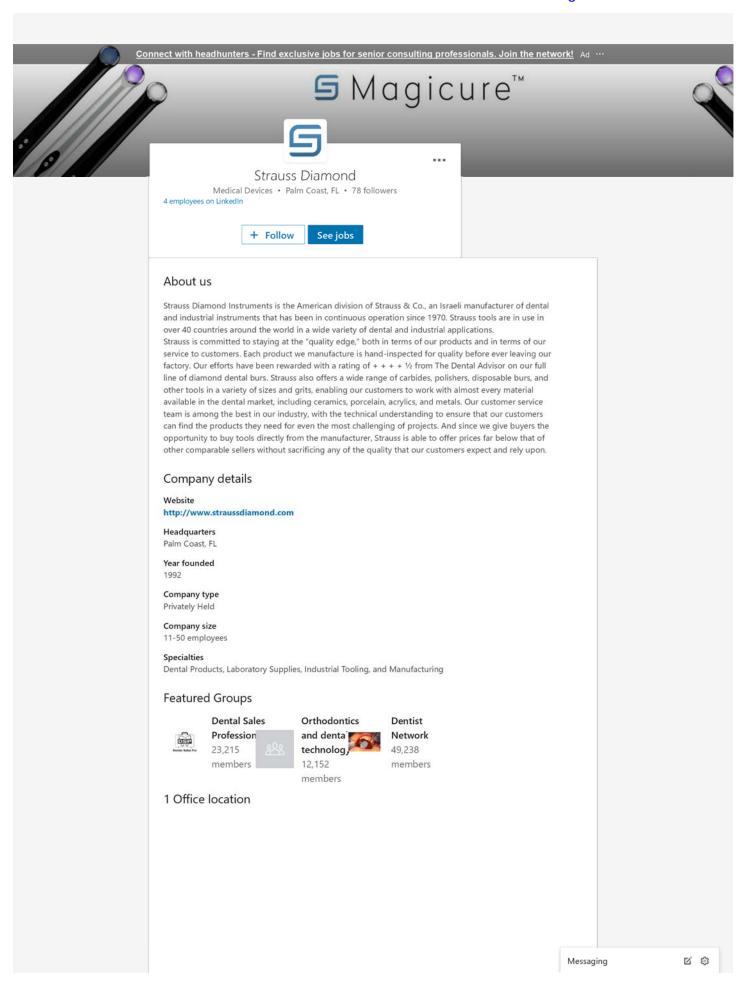

Case 3:18-cv-06663-TSH Document 22-16 Filed 01/24/19 Page 3 of 11

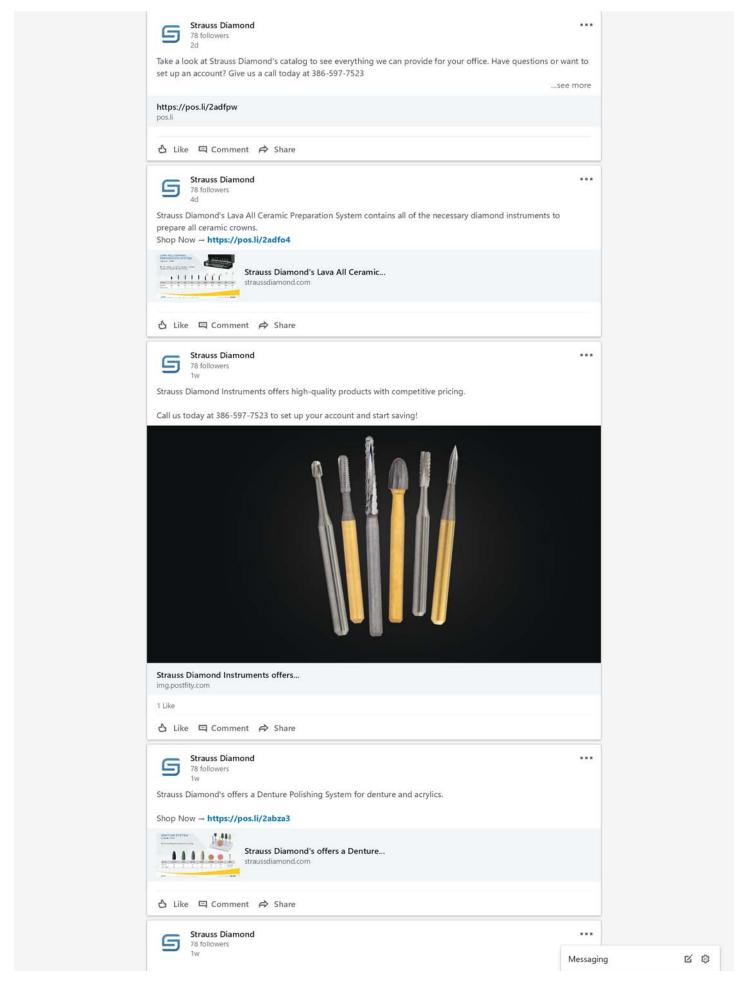

25% faster scanning time

Linkedin - with SD new scanner sleeve... 1507940147251-drlcss

0:00:40











0:01:19


Case 3:18-cv-06663-TSH Document 22-16 Filed 01/24/19 Page 5 of 11

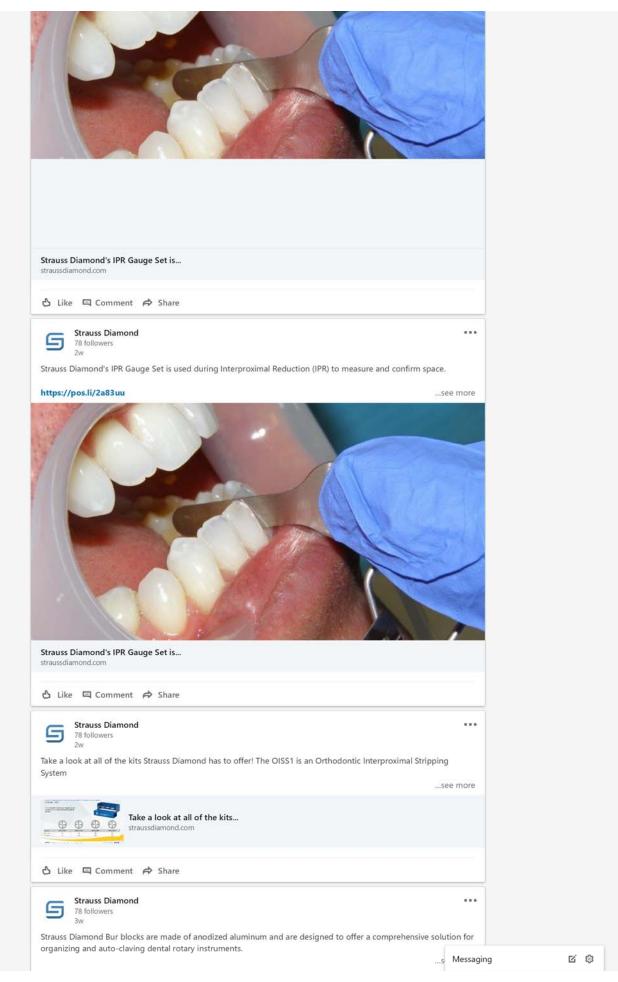


Case 3:18-cv-06663-TSH Document 22-16 Filed 01/24/19 Page 6 of 11

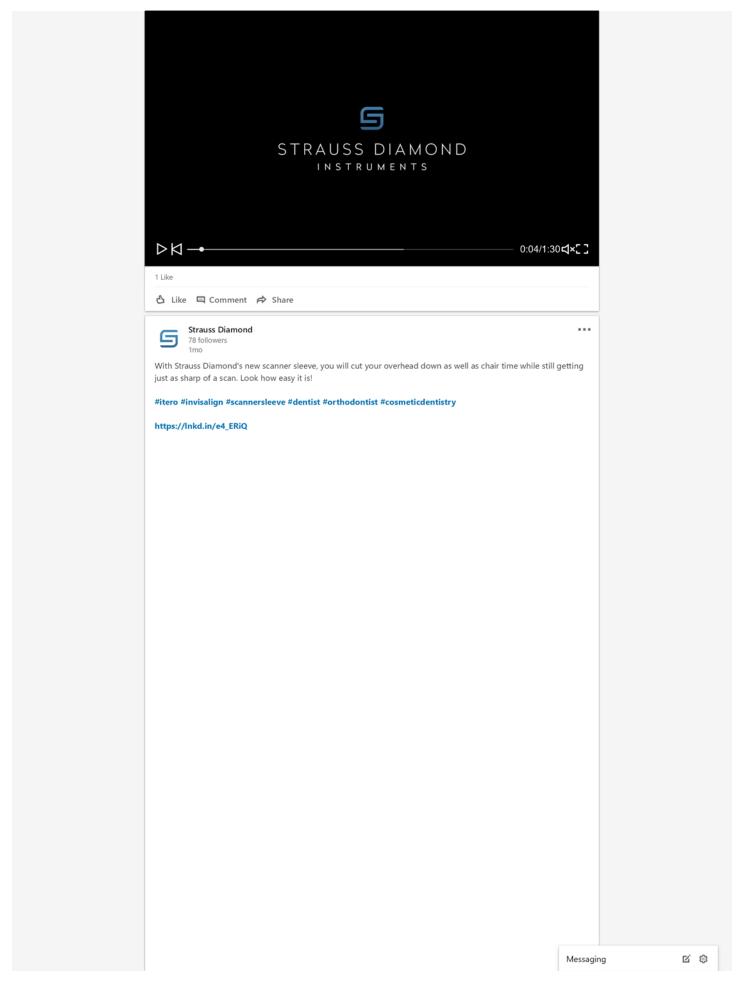

Case 3:18-cv-06663-TSH Document 22-16 Filed 01/24/19 Page 7 of 11

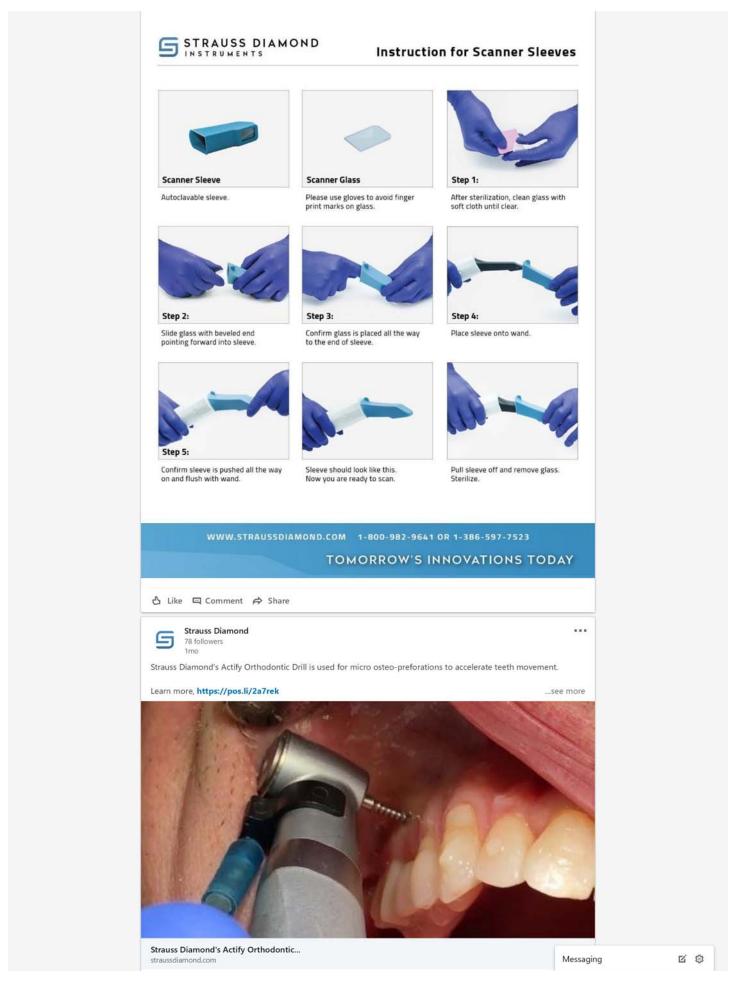

Case 3:18-cv-06663-TSH Document 22-16 Filed 01/24/19 Page 8 of 11

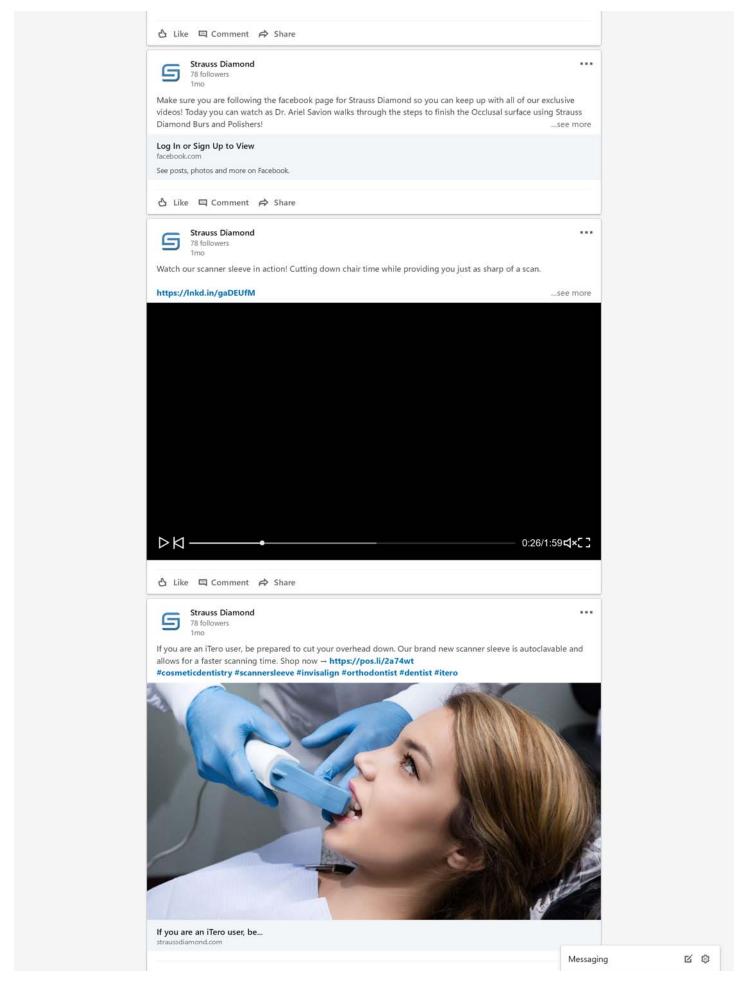

Case 3:18-cv-06663-TSH Document 22-16 Filed 01/24/19 Page 9 of 11

